



## Hoja de datos de Calibración de Prensa CBR

Fecha:	11/09/2016
Marca:	Soiltest
Modelo:	
Operador:	DO - PD

Hora:	10:00
Temp. (°C):	23
Rango:	0-3000kg
Apreciación:	5kg

1er ciclo


Prensa	Manómetro
0	21
105	119
205	218
300	304
400	393
500	494
600	585
700	683
800	779
900	875
1000	969
1100	1065
1200	1159
1300	1259
1400	1362
1500	1460
1600	1561
1700	1655
1800	1762
1900	1863
2000	1968
2100	2074
2200	2153
2300	2256
2400	2350
2500	2444
2600	2551
2800	2738
2900	2834
3000	2940
3300	3136
3400	3284
3500	3412

2do ciclo

Prensa	Manómetro
0	2
105	117
205	213
300	304
400	393
500	475
600	587
700	679
800	772
900	857
1000	969
1100	1072
1200	1166
1300	1259
1400	1362
1500	1463
1600	1552
1700	1657

3er ciclo

Prensa	Manómetro
-10	5
115	150
215	246
305	332
450	470
505	522
605	618
705	719
800	815
905	915
1010	1013
1100	1102
1210	1215
1310	1315
1420	1418
1535	1538
1630	1643
1730	1720

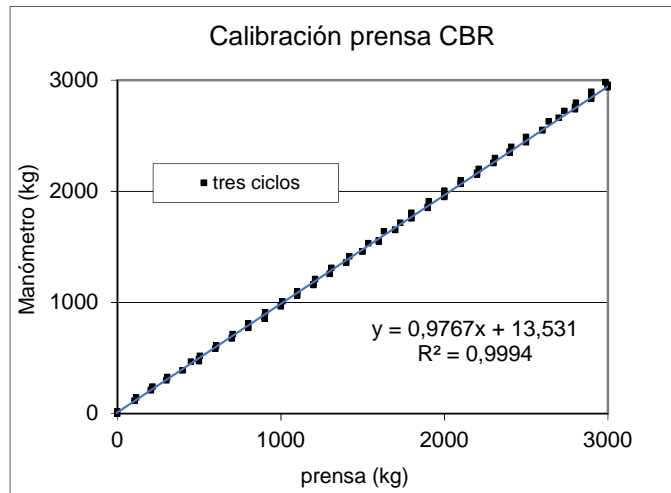

Manómetro digital Vegabar 53  
 VEGA  
 Code N° 516-962-10  
 Type BM1-47D-0/PD  
 Serial N° 1103497  
 Grade: 0

Revisado y aprobado por: